



CHT2014-10 批次 T₄ 檢驗院際品管統計分佈圖

送檢批號：CHT2014-10 檢體寄出日期：2014年10月01日 報告截止日期：2014年10月08日
 回收份數(比率)：21份(100%)



Sample S1

檢體 S1

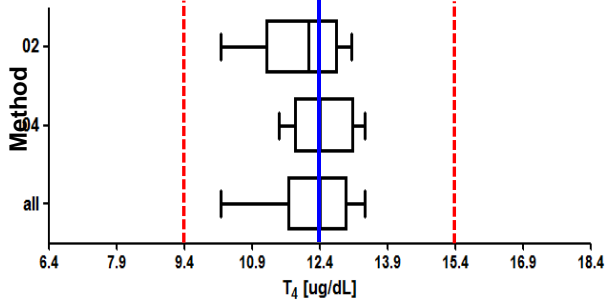


Method	檢驗單位數	中位值 (Median)	平均值 (Mean)	標準差 (SD)	變異係數 (CV)
02	8	12.2	12.0*	1.03*	8.6%
04	13	12.4	12.5*	0.77*	6.2%
All	21	12.4	12.3*	0.82*	6.7%
AEL**	117	12.0	12.2	1.49	12.2%

Certified assigned value : 12.4 µg/dL

Sample S2

檢體 S2

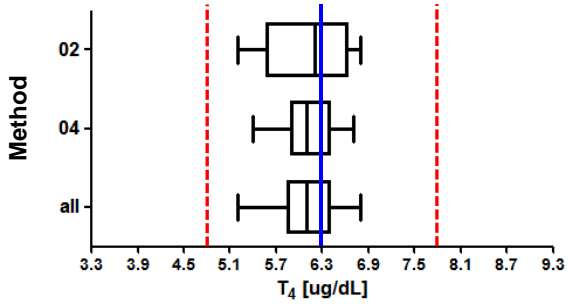


Method	檢驗單位數	中位值 (Median)	平均值 (Mean)	標準差 (SD)	變異係數 (CV)
02	8	6.2	6.1*	0.64*	10.5%
04	13	6.1	6.1*	0.44*	7.2%
All	21	6.1	6.1*	0.50*	8.2%
AEL**	117	6.2	6.3	0.82	13.0%


Certified assigned value : 6.3 µg/dL

* Calculated by robust method (ISO 13528 ; Algorithm A)
 ** All European Laboratories

* — Assigned value , - - - MAD

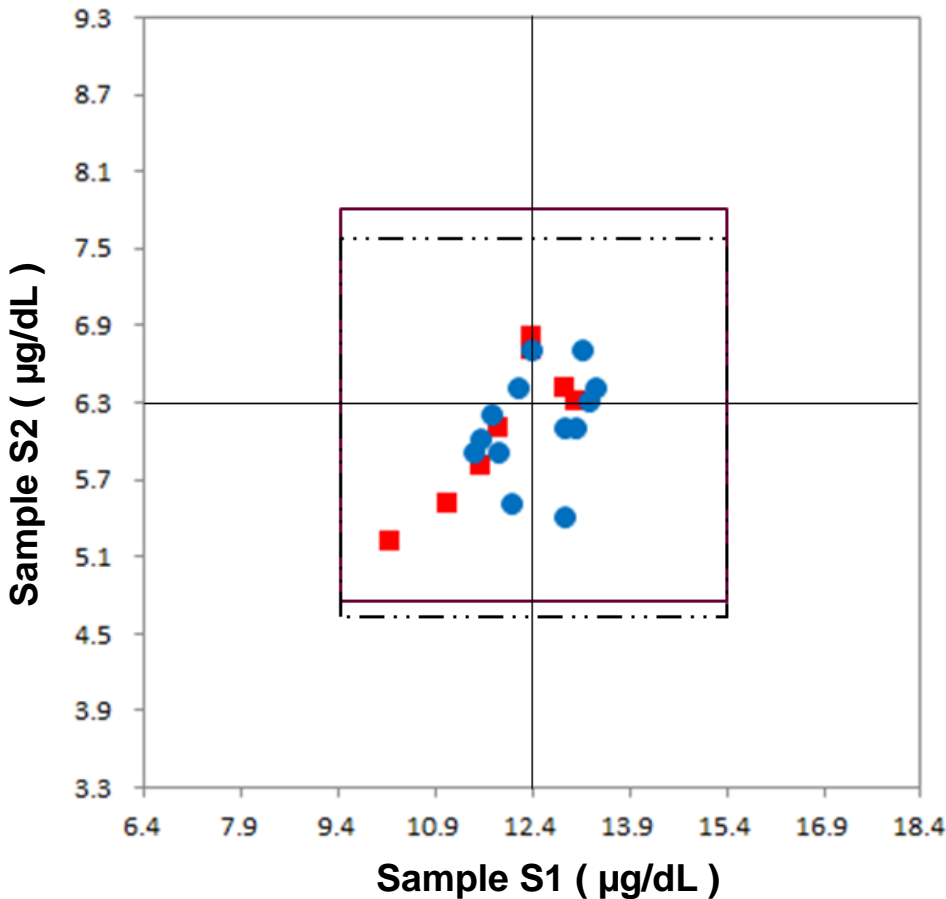

Youden Plot 圖例說明

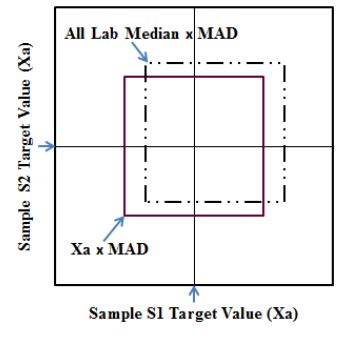

- Method 02 (RIA)
- Method 04 (CLIA)
- MAD : Maximum Allowable Deviation