



CHT2015-01 批次 T₃ 檢驗院際品管統計分佈圖

送檢批號：CHT2015-01 檢體寄出日期：2015年02月02日 報告截止日期：2015年02月09日


回收份數(比率)：21份(100%)



檢體 S1

Method	檢驗單位數	中位值 (Median)	平均值 (Mean)	標準差 (SD)	變異係數 (CV)
02	10	235	234*	19.6*	8.4%
04	11	263	262*	17.6*	6.7%
All	21	248	249*	28.6*	11.5%
AEL**	136	284	286	37.0	13.0%

Certified assigned value : 260 ng/dL



檢體 S2


Method	檢驗單位數	中位值 (Median)	平均值 (Mean)	標準差 (SD)	變異係數 (CV)
02	10	162	166*	21.9*	13.2%
04	11	218	224*	29.8*	13.3%
All	21	197	196*	41.3*	21.1%
AEL**	138	246	245	32.1	13.1%

Certified assigned value : 193 ng/dL


* Calculated by robust method (ISO 13528 ; Algorithm A)

** All European Laboratories

* — Assigned value , - - - MAD

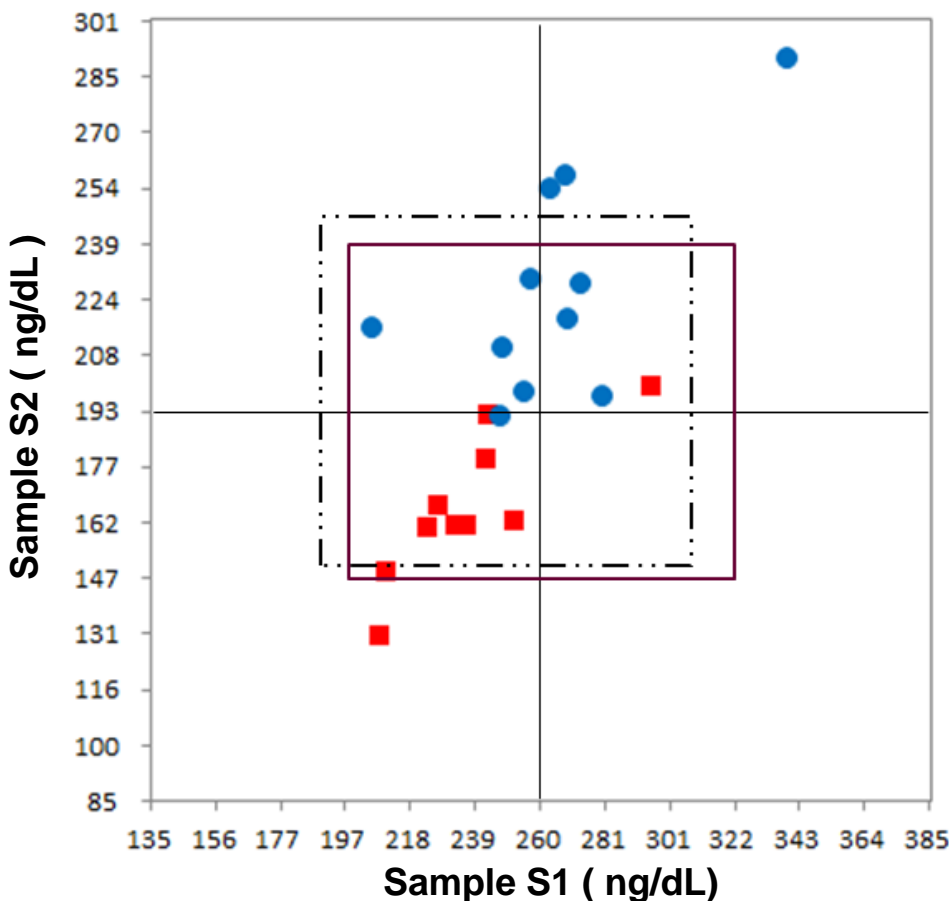

Youden Plot 圖例說明



■ Method 02 (RIA)

● Method 04 (CLIA)

MAD : Maximum Allowable Deviation