



CHT2015-01 批次 T₄ 檢驗院際品管統計分佈圖

送檢批號：CHT2015-01 檢體寄出日期：2015年02月02日 報告截止日期：2015年02月09日

回收份數(比率)：21份(100%)



Sample S1

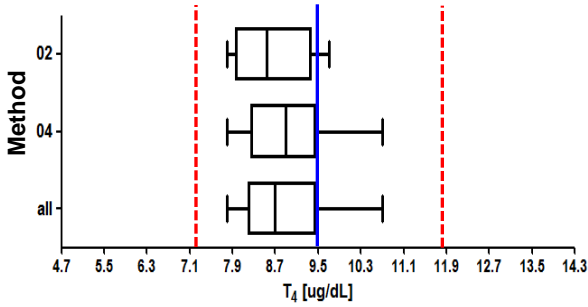


檢體 S1

Method	檢驗單位數	中位值 (Median)	平均值 (Mean)	標準差 (SD)	變異係數 (CV)
02	8	8.6	8.6*	0.80*	9.3%
04	13	8.9	8.9*	0.93*	10.4%
All	21	8.7	8.8*	0.82*	9.3%
AEL**	104	8.9	9.1	0.99	10.9%

Certified assigned value : 9.5 µg/dL

Sample S2

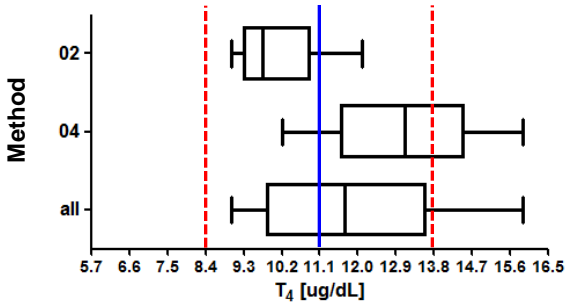

檢體 S2


Method	檢驗單位數	中位值 (Median)	平均值 (Mean)	標準差 (SD)	變異係數 (CV)
02	8	9.8	10.0*	1.04*	10.4%
04	13	13.1	13.2*	1.88*	14.2%
All	21	11.7	12.0*	2.39*	19.9%
AEL**	106	11.3	11.7	1.71	14.7%

Certified assigned value : 11.1 µg/dL


* Calculated by robust method (ISO 13528 ; Algorithm A)

** All European Laboratories

* — Assigned value , - - - MAD

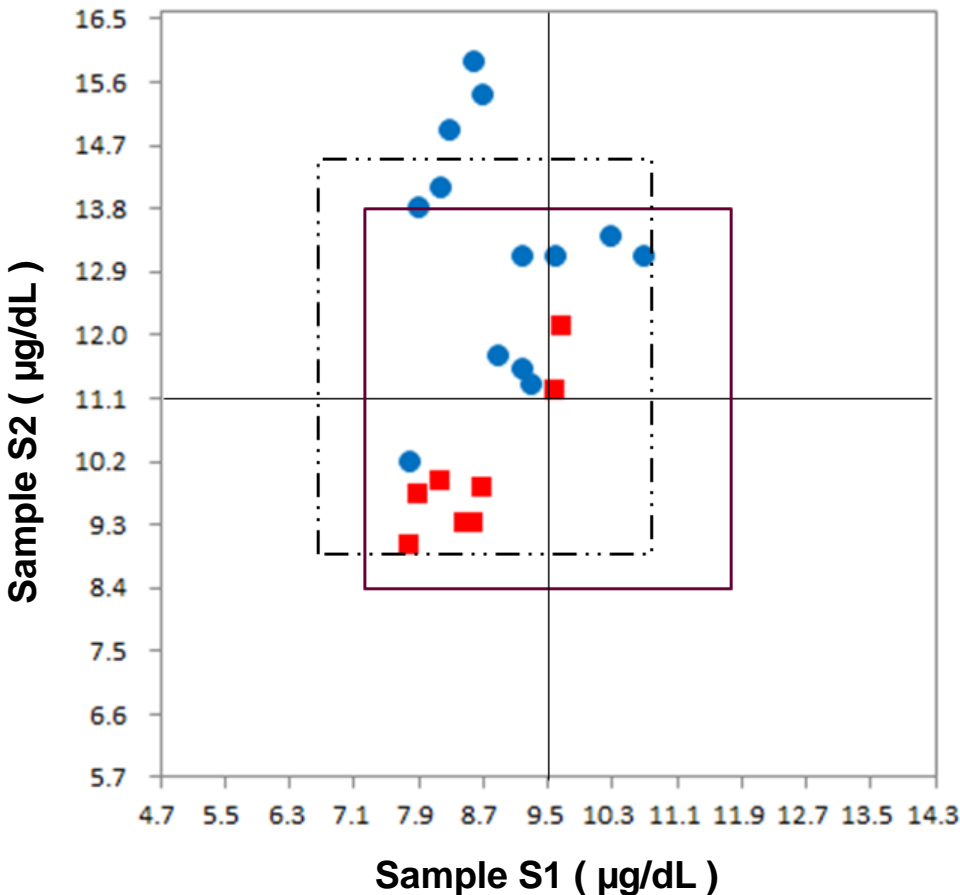

Youden Plot 圖例說明

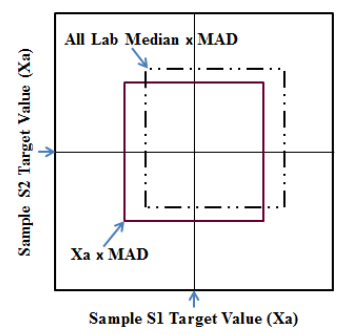

- Method 02 (RIA)
- Method 04 (CLIA)
- MAD : Maximum Allowable Deviation