



CHT2015-07 批次 T₄ 檢驗院際品管統計分佈圖

送檢批號：CHT2015-07 檢體寄出日期：2015 年 07 月 13 日 報告截止日期：2015 年 07 月 20 日

回收份數(比率)：21 份 (100%)



Sample S1

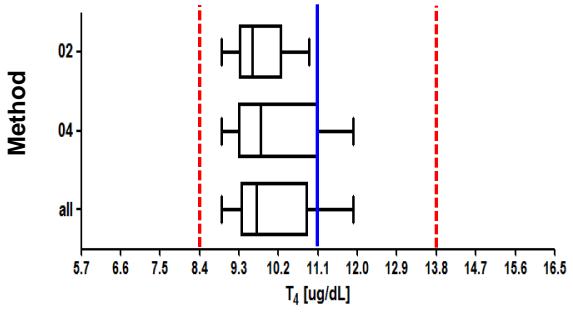


檢體 S1

Method	檢驗單位數	中位值 (Median)	平均值 (Mean)	標準差 (SD)	變異係數 (CV)
02	8	9.6	9.7*	0.69*	7.1%
04	13	9.8	10.2*	1.15*	11.3%
All	21	9.7	10.0*	0.94*	9.4%
AEL**	104	10.5	10.6	1.06	9.9%

Certified assigned value : 11.1 µg/dL

Sample S2

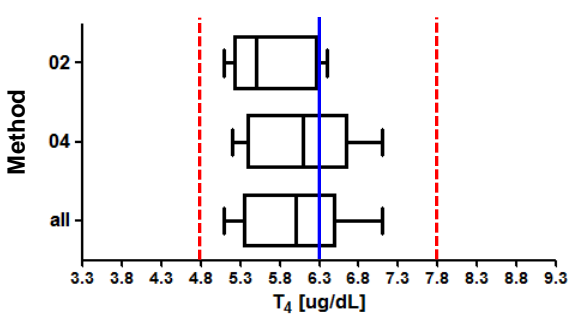

檢體 S2


Method	檢驗單位數	中位值 (Median)	平均值 (Mean)	標準差 (SD)	變異係數 (CV)
02	8	5.5	5.7*	0.60*	10.5%
04	13	6.1	6.1*	0.72*	11.8%
All	21	6.0	5.9*	0.69*	11.7%
AEL**	117	6.2	6.3	0.82	13.0%

Certified assigned value : 6.3 µg/dL


* Calculated by robust method (ISO 13528 ; Algorithm A)

** All European Laboratories

* — Assigned value , - - - MAD

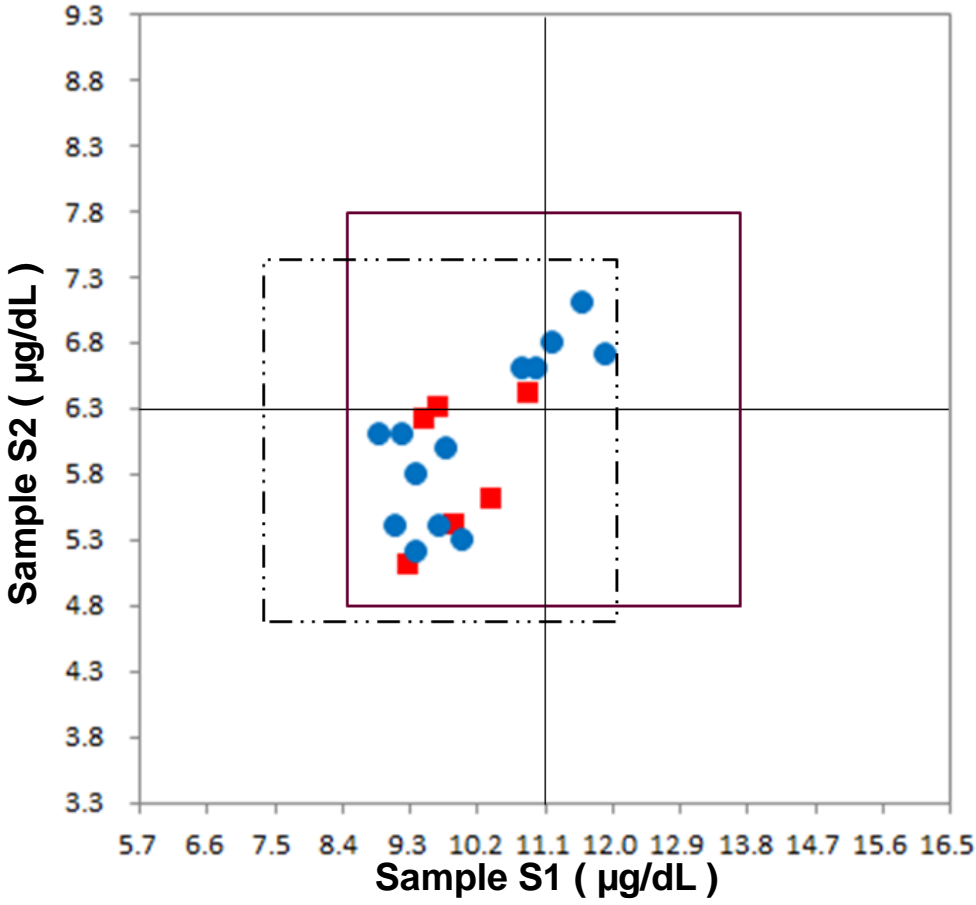

Youden Plot 圖例說明

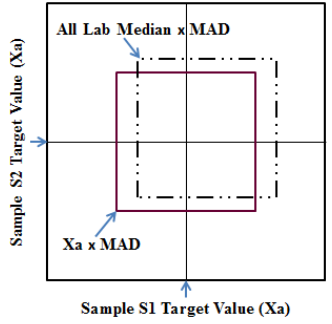

- Method 02 (RIA)
- Method 04 (CLIA)

MAD : Maximum Allowable Deviation